



# **Spectral-CT Phantom**

# The QRM-Spectral-CT Phantom was designed to test multi-energy spectral CT protocols and post processing techniques.

Image acquisition and image processing at multiple energy levels is improving visualization for computed tomography.

The Spectral-CT Phantom can be used to test different type of CT-machines with dual-energy, multi-energy or photon-counting setups.

The 100 mm cylinder contains 4 holes of 20 mm diameter to house different test rods of solid tissue equivalent materials or fillable rods that can be used with water or contrast media.

The phantom includes a set of different solid rods of lodine, Ca-hydroxyapatite, water and soft tissue equivalents as adipose, muscle, bone, and lung.

Mass density, electron density and effective atomic number (z) are given for each material.

#### **Features**

- Test the accuracy and consistency of spectral CT
- Test the Scanner performance
- Perform a material characterization and quantification of tissue equivalent materials
- Decompose iodine and Ca levels
- Test the post processing techniques of spectral CT

### Part list of QRM-SCT

- Water equivalent cylinder with 4 bores
- 4 plugs CTWater® (0 HU @ 70 150 kV)
- 12 test rods:

adipose tissue (ICRU 44) muscle tissue (ICRU 44)

lung tissue (ICRU 44)

liver tissue (ICRU 44)

4 different lodine rods (CTlodine®)\*

2, 5, 10 and 15 mg I/cm<sup>3</sup>


4 different Ca-HA rods (Bone)

100, 200, 400 and 800 mg HA/cm<sup>3</sup>

2 fillable rods/tubes



Spectral-CT Phantom

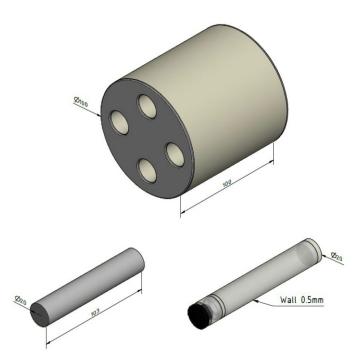

Phantom dimensions, D100 cylinder, ICRU rods and fillable rods



D100: fits also into 深圳市展业达鸿科技有限公司:tom


吕先生:15920060912(微信同号) 0755-22934005(座机)

地址:深圳市福田区八卦二路八卦岭工业区615栋419


邮箱:hongqi@thingstet.com 网址:www.thingstest.com



# **Spectral-CT Phantom**

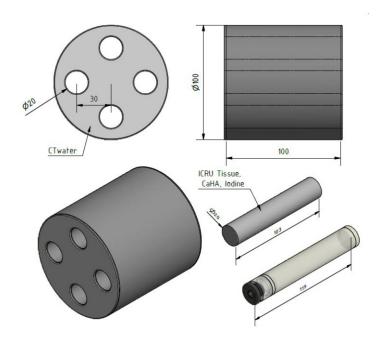

Schematic view of the DE-Phantom

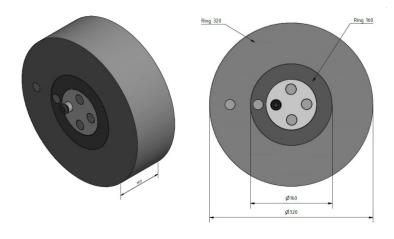

QRM-SCT with optional rings D160 and S320

## **Specifications**

Phantom diameter	100 mm
Phantom length	103 mm
Phantom weight	. 1.0 kg
Rod diameter	20 mm
Rod length	103 mm

## Optional available


Ring 160	CTWATER® D160mm / H100, bore 20	0
Ring 320	CTWATER® D320mm / H100, bore 20	0
Additional Rods	Tissue equivalents ICRU 44/46 Iodine, CaHA	
Tubes	Fillable rods	
Cylinder	CTWATER® D100 mm 8 holes	
Abdomen	200 x 300 mm H 100	Conc

<sup>\*</sup>specified values. Nominal values can vary with respect to manufacturing method and imaging device!

#### **References:**

[1] Ehn S, Sellerer T, Noel P, et al.

Assessment of quantification accuracy and image quality of a full-body dual-layer spectral CT system



吕先生:15920060912(微信同号) 0755-22934005(座机)

地址:深圳市福田区八卦二路八卦岭工业区615栋419

邮箱:hongqi@thingstet.com 网址:www.thingstest.com